

Proceq Europe

Ringstrasse 2
8603 Schwerzenbach
Switzerland
Phone +41-43-355 38 00
Fax +41-43-355 38 12
info-europe@proceq.com

Proceq UK Ltd.

Bedford i-lab, Priory Business Park
Stannard Way
Bedford MK44 3RZ
United Kingdom
Phone +44-12-3483-4515
info-uk@proceq.com

Proceq USA, Inc.

117 Corporation Drive
Aliquippa, PA 15001
U.S.A.
Phone +1-724-512-0330
Fax +1-724-512-0331
info-usa@proceq.com

Proceq Asia Pte Ltd

12 New Industrial Road
#02-02A Morningstar Centre
Singapore 536202
Phone +65-6382-3966
Fax +65-6382-3307
info-asia@proceq.com

Proceq Rus LLC

Ul.Optikov 4
korp.2, lit. A, Office 321
197374 St. Petersburg
Russia
Phone/Fax +7 812 448 35 00
info-russia@proceq.com

Proceq Middle East

P.O. Box: 262419
Jebel Ali Free Zone
Dubai, United Arab Emirates
Phone +971 50 482 9510
info-middleeast@proceq.com

Proceq SAO Ltd.

South American Operations
Rua Haddock Lobo, 746 - 5 andar
Cerqueira Cesar, São Paulo
Brasil Cep. 01414-000
Phone +55 11 3083 38 89
info-southamerica@proceq.com

Proceq China

Unit G, 10th Floor, Huamin •Empire Plaza
No. 728, Yan An Road(W)
Shanghai, 200050
China
Phone +86 21-63177479
Fax +86 21 63175015
info-china@proceq.com

**proceq**

Operating Instructions

Shear Wave Transducers 250 kHz

proceq

Required steps before measurements can be performed

1. Put a small amount of shear wave coupling gel on the transducers.
2. Firmly press the transducers on either side of the 25 μs calibration rod (Part No 710 10 028). Make sure that the coupling gel is properly distributed and that no air is trapped between the transducer and the calibration rod.
3. Connect the transducers to Pundit Lab.
4. Select the 250 kHz transducer from the list of supported transducers (see Pundit Lab manual chapter 3 for more details).
5. Zero the instrument as described in the Pundit Lab manual chapter 2.1.

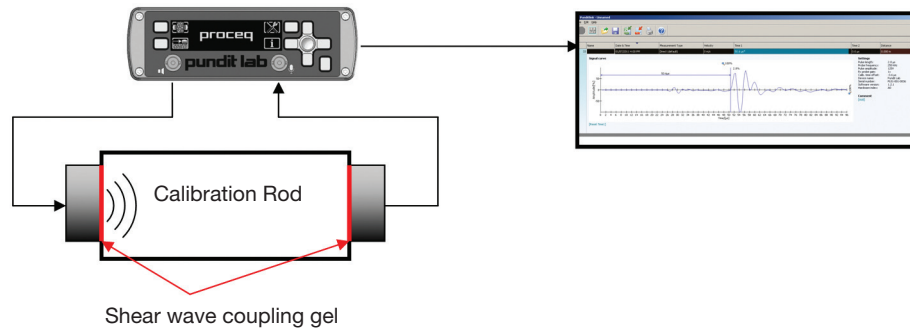


Figure 1: Performing measurements with the 250 kHz shear wave transducers.

Performing measurements (see Figure 1)

When measurements with the 250 kHz shear wave transducers are performed, it is crucial to use the special shear wave coupling paste, otherwise shear waves cannot be properly transmitted into the object under test. The shear wave coupling paste is a non-toxic, water soluble organic substance of very high viscosity.

Furthermore, we highly recommend using Pundit Link's waveform display in order to manually locate the onset of the shear wave echo. Since the latter is always preceded by a relatively weak longitudinal echo (see Figure 2), the transit time determined by Pundit Lab, would correspond to the longitudinal instead of the shear wave.

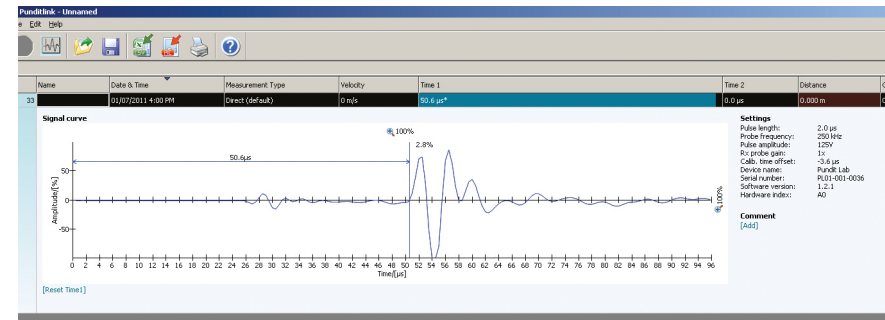


Figure 2: Typical echo signal obtained, with an experimental setup according to figure 1.

The first echo arrives at approximately 25.4 μs and corresponds to the weak longitudinal wave generated by the shear wave transducer. After 50.6 μs the much stronger shear wave echo appears in the signal.